

AB Tip İnceleme Sertifikası EU Type-Examination Certificate

Belge No / Certificate No : 161-21-02

Belgelendirme Tarihi - Bir Sonraki Belge Tarihi /

Certification Date / Certificate Validity Date : 02.04.2021-02.04.2026

Belge Geçerlilik Tarihi / Document Validity Period: 5 yıl / 5 years

Firma Unvanı ve Adresi /

Company Name and Address

: COOL AGENCY SRO

Koněvova 2660/141, Žižkov (Praha 3), 130

00 Praha, Zizkov

Ürün Adı /Modeller / Product Name / Models Direktifi / Directive

Modülü/Kategori / Module / Category

: PROMEDOR 24 FFP2 NR PRIMUS XXS

: 2016/425 REGULATION

: B MODÜLÜ/ KATEGORİ III MODULE B / CATEGORY III

: MNA M-2020-000405

Test Rapor No/ları / Test Report No Ürün Tipi / Product Type:

> EN 149:2001+ A1:2009 Solunumla ilgili koruyucu cihazlar - Parçacıklara karşı koruma amaçlı filtreli yarım maskeler/ Respiratory protective devices - Filtering half masks to protect against particles

Ürünün Malzeme Bilgisi / Product Material Information: PROMEDOR 24 FFP2 NR PRIMUS XXS model ürünleri kumaş, elatik kayışı, burun klipsi, filtre katmanı kullanılarak imal edilmiştir./ PROMEDOR 24 FFP2 NR PRIMUS XXS model products are manufactured using fabric, elastic strap, nose clip, filter layer.

Volkan AKIN 02.04.2021 Karar Verici / Approver Okan AKEL 02.04.2021 Şirket Müdürü / General manager










ATTACHMENTS (161-21-02)

To certify the PPE product at Category III level, C2 or D module is accompanied by applying one of the conformity assessment methods along with the EU Type Examination (Module B).

Model: PROMEDOR 24 FFP2 NR PRIMUS XXS

PPE SPECIFICATION	PERFORMANCE LEVELS
Classification	FFP2
Reusable / Single Shift Use	NR


PPE produced as a single unit to fit an individual user, all the necessary instructions for manufacturing such PPE on the basis of the approved basic model:

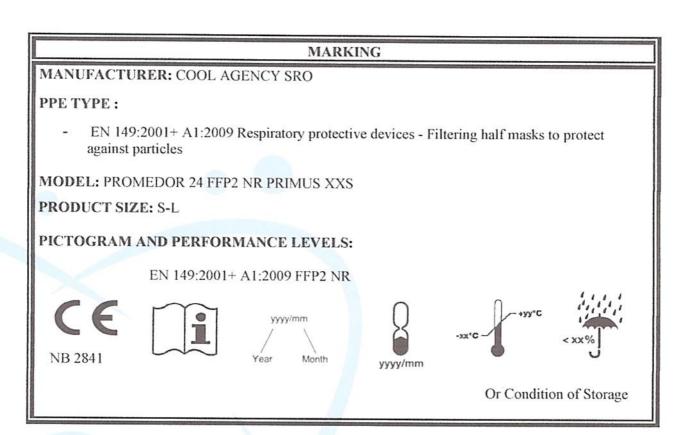

MNA LABORATORIES SAN. TIC. LTD. \$TI declares that the above-mentioned product meets the requirements of the directive according to the EU Directive 2016/425, the safety of the product is covered by the conditions and use specified in this certificate and in the technical file.



ATTACHMENTS (161-21-02)

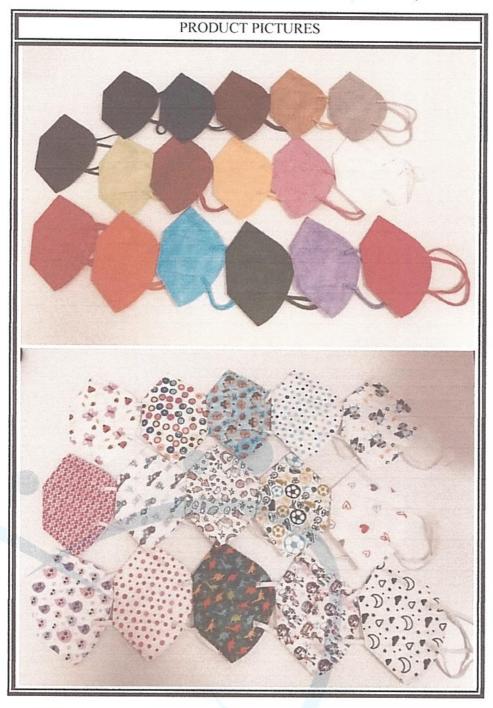



ATTACHMENTS (161-21-02)



DOCUMENTS IN THE TECHNICAL FILE

- Basic Health Safety Requirements
- Risk Assessment
- Test Reports
- Technical Report



TECHNICAL EVALUATION REPORT (161-21-02)

Report No : 161-21-02

Report Date : 02.04.2021

Application No : 161-21-02

1. COMPANY INFORMATION:

COOL AGENCY SRO

Koněvova 2660/141, Žižkov (Praha 3), 130 00 Praha, Zizkov

Tel: +90 532 135 05 79

2. PPE INFORMATION:

Disposable and non-sterile half mask made of particulate protection fitler material.

3. PPE TYPE IDENTIFICATION

EN 149:2001+A1:2009 Respiratory protective devices – Filtering half masks to protect against particles - Requirements, testing, marking

4. PPE PICTURES







TECHNICAL EVALUATION REPORT (161-21-02)



PROMEDOR 24 FFP2 NR PRIMUS XXS

5. PPE DIMENSIONS:

PROMEDOR 24 FFP2 NR PRIMUS XXS model has been found to be produced using S-L sizes.

6. PPE PRODUCT MATERIAL INFORMATION:

The product is made of elastic strap, nonwoven fabric on the outer and inner layers and fitler material on the middle layer.

7. ESSENTIAL HEALTH AND SAFETY REQUIREMENTS

- A visual inspection was made according to EN 149:2001 +A1:2009 for ergonomics.
- Protection levels and degrees are defined by the manufacturer.
- Suitable construction materials were determined by visual inspection according to EN 149:2001 +A1:2009.

8. ANALYSIS AND EVALUATIONS:

EN 149:2001 +A1:2009

TESTS	PARAMETER PERFORMANCE LEVELS			RESULTS	PERFORMANCE LEVELS	EVALUATION	
		FFP1	FFP2	FFP3			
Part 7.3 Visual inspection	Shall also the mark supplied by the mar			mation	Appropriate	-	PASS
Part 7.4 Packaging	for sale packaged are protected agai	icle filtering half mask shall be offered sale packaged in such a way that they protected against mechanical damage contamination before use.			Appropriate	-	PASS
Part 7.5 Material	The state of the s	hen conditioned in accordance 8.3.1 & 3.2 the particle filter half mask shall not			Appropriate	-	PASS
Part 7.6 Cleaning and		disinfecting the re-usable			Not applicable	-	Not applicable



TECHNICAL EVALUATION REPORT (161-21-02)

disinfecting	penetration requirement of the relevant class.			
Part 7.7 No negative comments should be made by the test subject regarding any of the criteria performance evaluated.		Appropriate	-	PASS
Part 7.8 Finish of parts	Parts of the device likely to come into contact with the wearer shall have no sharp edge or burrs.	Appropriate	-	PASS
Banned Azo Dyes	< 30 mg/kg	< 5 mg/kg	< 30 mg/kg	PASS

TESTS PARAMETER	PARAMETER	PERFORMANCE LEVELS		RESULTS	PERFORMANCE LEVELS	EVALUATION	
		FFP1	FFP2	FFP3		and the second of the second o	
Part 7.9.1 Total inward leakage	At least 46 out of the 50 individual exercise result	<25	<11	<5	See the table below	FFP2	PASS
	At least 8 out of the 10 individual wearer arithmetic means	<22	<8	<2	See the table below	FFP2	PASS

	Total Inwar	d Leakage (%	6)			
	Exercise 1	Exercise 2	Exercise 3	Exercise 4	Exercise 5	Average
Subject 1 (As recieved)	6.2	5.9	5.5	7.8	7.9	6.7
Subject 2 (As recieved)	5.7	6.1	4.9	8.0	7.8	6.5
Subject 3 (As recieved)	7.0	6.0	7.6	7.2	7.6	7.1
Subject 4 (As recieved)	6.7	7.7	7.5	8.9	7.8	7.7
Subject 5 (As recieved)	6.4	7.9	8.2	3.8	7.8	6.8
Subject 6 (After temperature conditioning)	6.3	7.0	6.8	6.3	7.8	6.8
Subject 7 (After temperature conditioning)	6.1	7.3	6.7	7.6	6.2	6.8
Subject 8 (After temperature conditioning)	6.4	6.7	6.4	7.8	7.7	7.0
Subject 9 (After temperature conditioning)	6.4	6.6	6.3	7.6	6.2	6.6
Subject 10 (After temperature conditioning)	6.3	7.4	7.6	7.4	6.2	7.0

Subject facial dimensions

Subject	Face Length (mm)	Face Width (mm)	Face Depth (mm)	Mouth Widtl (mm)	
1	133	132	132	65	
2	125	144	116	67	
3	126	135	124	75	
4	4 123		134	74	
5	117	135	122	73	
6	122	142	133	66	
7	113	132	114	75	
8	135	123	123	65	
9	122 135		133	74	
10	135	142	125	83	



TECHNICAL EVALUATION REPORT (161-21-02)

TESTS PARAMETER	PARAMETER	PERFORMANCE LEVELS		RESULTS	PERFORMANCE LEVELS	EVALUATION	
	FFP1	FFP2	FFP3				
Part 7.9.2 Penetration of filter	Sodium chloride, 95 L/min %, max	% 20	% 6	%1	See the table below	FFP2	PASS
material	Paraffin oil, 95 L/min %, max	% 20	% 6	%1	See the table below	FFP2	PASS

Penetration of filter material	Sodium Chloride (%)	Paraffin Oil (%)	
As recieved	3.6	3.9	
As recieved	3.5	4.5	
As recieved	4.1	4.1	
After the simulated wearing treatment	3.6	4.0	
After the simulated wearing treatment	3.3	4.2	
After the simulated wearing treatment	3.0	4.6	
Mechanical strength and temperature conditioning	4.9	5.0	
Mechanical strength and temperature conditioning	5.1	5.1	
Mechanical strength and temperature conditioning	5.0	5.4	

TESTS	PARAMETER	PERFC	RMANO	CE LEVELS	RESULTS	PERFORMANCE	EVALUATION	
			FFP2	FFP3		LEVELS		
Part 7.10 Compatibility with skin	Materials shall not be cause irritation or an health			-	Appropriate	-	PASS	
Part 7.11 Flammibility	Mask shall not burn o for more than 5 s	r not to	continu	e to burn	Flame not seen	-	PASS	
Part 7.12 Carbondioxide content of the inhalation air	Shall not exceed an av	erage o	f % 1		0,69 0,67 0,68	-	PASS	
Part 7.13 Head harness	It can be donned and	remove	d easily		Appropriate	-	PASS	
Part 7.14 Field of vision	The field of vision sha performance test.	all accep	table in	practical	Appropriate	-	PASS	
Part 7.15 Exhalation valve(s)	It shall withstand axia apply for 10 s. If fitted, shall continuafter a continuous L/min over a period of	ue to c	perate	correctly	Not applicable	-	Not applicable	
TESTS	PARAMETER	PERFO FFP1	PERFORMANCE LEVELS		RESULTS	PERFORMANCE LEVELS	EVALUATION	
Part 7.16 Breathing	Inhalation 30L/min	0,6 mbar	0,7 mbar	1,0 mbar	See the table below	FFP2	PASS	
Resistance	Inhalation 95L/min	2,1 mbar	2,4 mbar	3,0 mbar	See the table below	FFP2	PASS	
	Exhalation 160L/min	3,0 mbar	3,0 mbar	3,0 mbar	See the table below	FFP2	PASS	



TECHNICAL EVALUATION REPORT (161-21-02)

Breathing Resistance (mbar)	Inhalation 30L/min	Inhalation 95L/min
As recieved	0.4	2,3
As recieved	0.3	2,2
As recieved	0.3	2,2
After temperature conditioning	0.4	2,3
After temperature conditioning	0.3	2,3
After temperature conditioning	0.4	2,3
After the simulated wearing treatment	0.4	2,2
After the simulated wearing treatment	0.3	2,3
After the simulated wearing treatment	0.4	2,3

Breathing Resistance 160L/min (mbar)	Facing directly ahead	Facing vertically upwards	Facing vertically downwards	Lying on the left side	Lying on the right side
As recieved	2,5	2,5	2,5	2,5	2,5
As recieved	2,5	2,6	2,5	2,5	2,6
As recieved	2,5	2,5	2,6	2,5	2,6
After temperature conditioning	2,6	2,5	2,6	2,5	2,5
After temperature conditioning	2,5	2,5	2,5	2,5	2.5
After temperature conditioning	2,5	2,5	2,5	2,6	2,5
After the simulated wearing treatment	2,5	2,5	2,5	2,5	2,6
After the simulated wearing treatment	2,6	2,5	2,6	2,5	2,5
After the simulated wearing treatment	2,5	2,5	2,5	2,6	2,5

TESTS	PARAMETER	PARAMETER PERFORMANCE LEVELS				PERFORMANCE LEVELS	EVALUATION
		FFP1	FFP2	FFP3			
Part 7.17 Clogging	After clogging the inhalation resistances shall not exceed. (valved)	4 mbar	5 mbar	7 mbar	Not applicable	-	Not applicable
	The exhalation resist 3 mbar at 160 L/ (valved)				Not applicable	-	Not applicable
	After clogging the inhalation and exhalation resistances shall not exceed. (valveless)	on and mbar mbar mbar ion aces shall exceed.				-	Not applicable
Part 7.18 Demountable part	All demountable par readily connected possible by hand.		anacharan ka ga		Not applicable	-	Not applicable

TECHNICAL EVALUATION REPORT (161-21-02)

9. DECISION PROPOSAL

Analysis and examinations PROMEDOR 24 FFP2 NR PRIMUS XXS model coded personal protective equipment; Respiratory Protective Devices EN 149:2001 +A1:2009- Filtered Half Masks for Protection Against Particles -Properties, Experiments and Marking standards are evaluated. It is recommended to be certified at the performance levels specified as a result of technical evaluations.

10. ATTACHMENTS

- Basic Health Safety Requirements
- Risk Assessment
- **Test Reports**
- **User Instruction**

CONTROLLER

: VOLKAN AKIN 2021 C

SING

DATE